

DuoDERM® Signal dressing – time to change



Designed to simplify wound management

- Visually indicates when to change the dressing*
- Flexible and conformable
- Translucent enhancing visual access to wound

Designed to stay in place

- Tapered border edges
- Low profile
- Smooth, low-friction film backing
- Designed to reduce premature dressing changes
- Designed to reduce the potential for dressing edges to ruck

Designed for use on acute and chronic wounds

- Leg ulcers
- Pressure ulcers
- Diabetic foot ulcers
- Partial thickness burns
- Post-operative wounds

ConvaTec Wound Therapeutics™
Helpline Freephone: 0800 289 738 (UK)
1800 946 938 (ROI)
Visit the ConvaTec website at:
www.convatec.com

DuoDERM® Signal is available as:

Square dressings

Size	Dressings/box	Order code
10 x 10cm	5	S166
14 x 14cm	5	S167
20 x 20cm	5	S168

Hip/shoulder dressing

Size	Dressings/box	Order code
11 x 19cm 	5	S174

Sacral dressing

Size	Dressings/box	Order code
22.5 x 20cm 	5	S170

Heel dressing

Size	Dressings/box	Order code
18.5 x 19.5cm 	5	S169



ConvaTec Wound Therapeutics™



'Life-enhancing products and services'

Good science and sound research are just part of the ConvaTec way. Healthcare is about more than clinical effectiveness, it's about making a difference to the way people live and work each day. That's why our approach to wound care looks beyond the laboratory to understand the needs of physicians, nurses, and those they care for. It's why so many trust us and our products.

Time to change

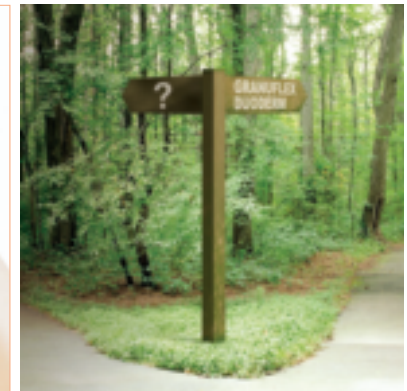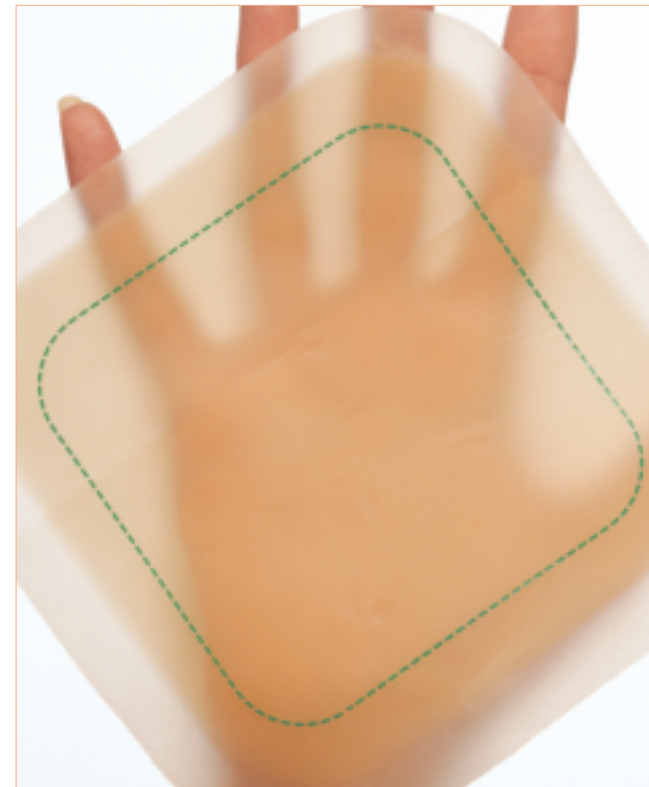

* The dressing should be changed when: clinically indicated when strike through occurs, or up to a maximum of 7 days. The wound should be cleansed at appropriate intervals.



SIMPLIFYING WOUND MANAGEMENT

– see for yourself

DuoDERM® Signal dressing provides a simple visual indication of when it's **time to change** the dressing*

- **Innovative visual indicator** helps determine accurate size selection of dressing and guides positioning
- **Designed to reduce premature dressing changes** that can disturb healing and cause discomfort



As DuoDERM® Signal dressing absorbs wound exudate, it forms a gel that may be visible as a bubble underneath the surface of the dressing. If the bubble expands to any part of the DuoDERM® Signal dotted dressing change indicator line, it is **time to change** the dressing.^{†,‡}

* The dressing should be changed when: clinically indicated when strike through occurs, or up to a maximum of 7 days. The wound should be cleansed at appropriate intervals.


† The bubble may not be visible with minimal exudate. If this occurs, the recommended maximum wear time is up to 7 days.

‡ Trimming the dressing may impair the function of the visual change indicator.

ENHANCING PATIENT COMFORT

DuoDERM® Signal dressing is designed to stay in place

- **Tapered border edges** help reduce the potential for dressing edges to catch against bed linen and clothing, enhancing patient comfort by reducing rucking
- **Smooth, low-friction film** backing helps reduce shear that can cause dressing to peel off
- **Low profile** makes dressing flexible and conformable
- **Anatomically designed shapes** (heel, sacral and oval) for hard-to-dress areas

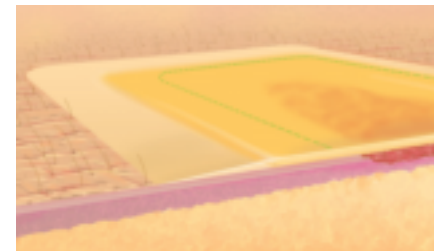

Tapered border edges help reduce the potential for dressing edges to catch against bed linen and clothing



Translucent to enhance visual access to the wound